

WYCENA DOTYCZĄCA ŚRODKA TECHNICZNEGO NR 37/XII/17

Dla: Powiatowy Szpital im. Wm Biegańskiego

ul. Andersa 3

14-200 Iława

1. Dane dotyczące środka technicznego:

Nazwa		Typ		
Aparatura endoskopowa STORZ monitor SONY		3-20113120		
		4-263310 20		
		2-20212020		
		5-264305 20		
		Silniki		
Nr fabryczny	Rok budowy	Oznaczenie	Numer	Moc
3-MN527	3-brak	Nie dotyczy	-----	-----
4-6002986	4 -brak			
2-brak	2-brak			
5-0002011	-brak			

Opis stanu technicznego: Stan techniczny maszyny określam jako dostateczny, wycofany z eksploatacji z bloku operacyjnego. W skład aparatury wchodzi: monitor, kamera z przetwornikiem -2, źródło światła-3, pompa płynów-4, pompa gazu-5

2. 3 Stopień zużycia technicznego szacuję (S)= 60%






4 Wskaźnik nowoczesności konstrukcji przyjmuję (K= 0,6)



5. Współczynnik urynkowienia E=0,5

Nie wyszukałem żadnych ofert w internecie, zatem wartość określam metodą odtworzeniową wg formuły $C = W \times / 1 - S / x K \times E$ W-w g. zleceniodawcy= 173352,21 zł Zatem


$$C = 173352,21 / 1 - 0,6 / x \times 0,6 \times 0,5 = 20\ 802\ \text{zł po zaokrągleniu}$$


9

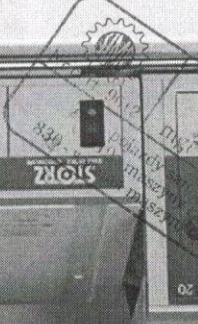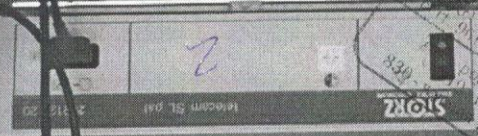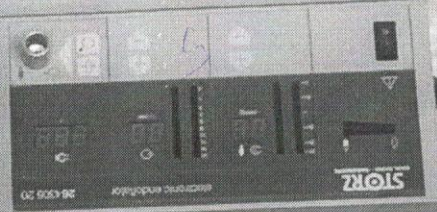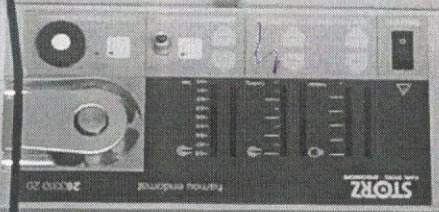
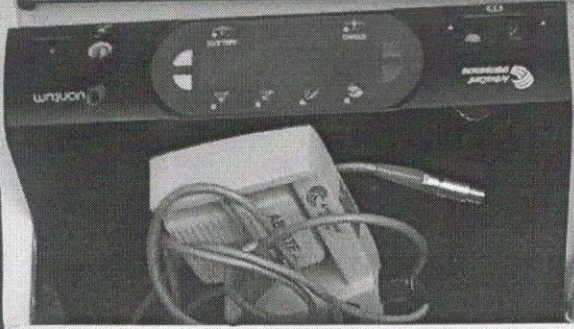


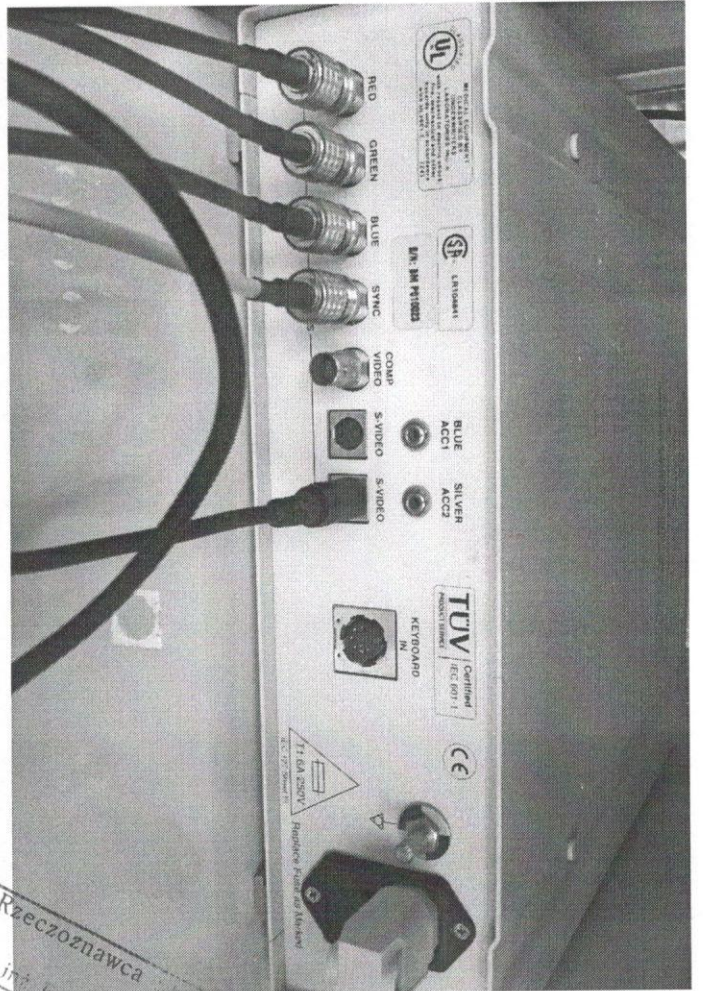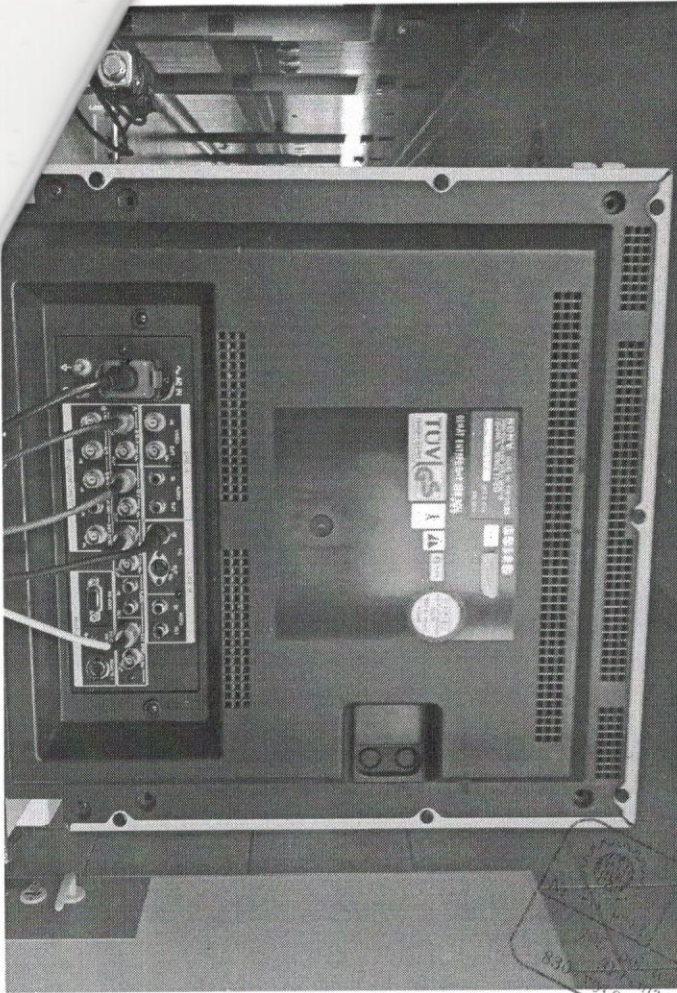

Rzeczoznawca
Franciszek Czerwik
830-000-0000
specjalista w dziedzinie maszyn rolniczych i ciągników
specjalista w dziedzinie maszyn, urządzeń i pojazdów

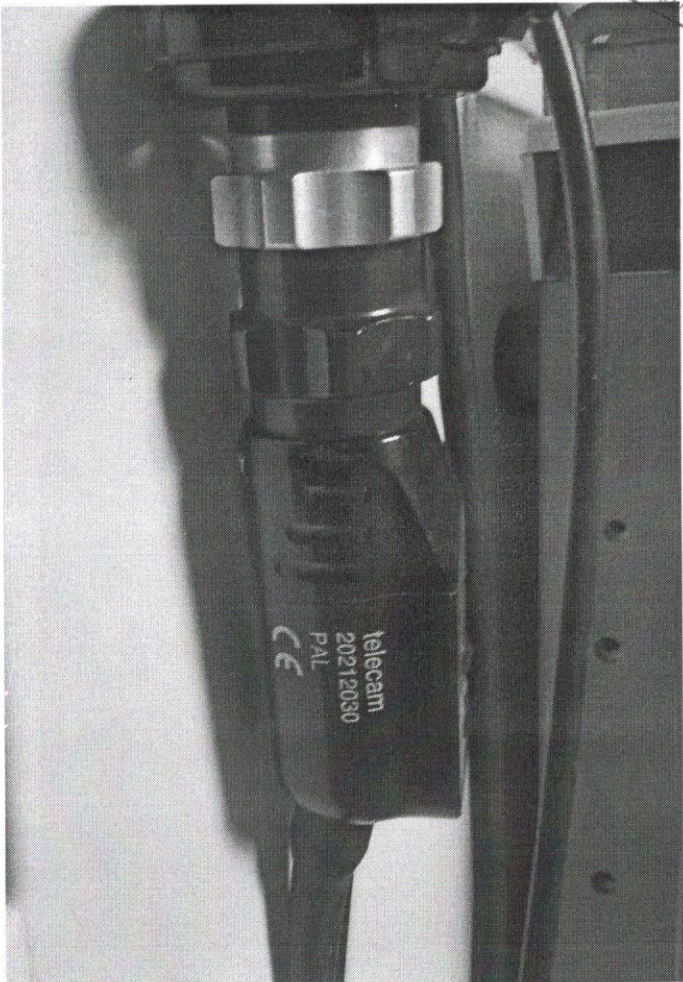

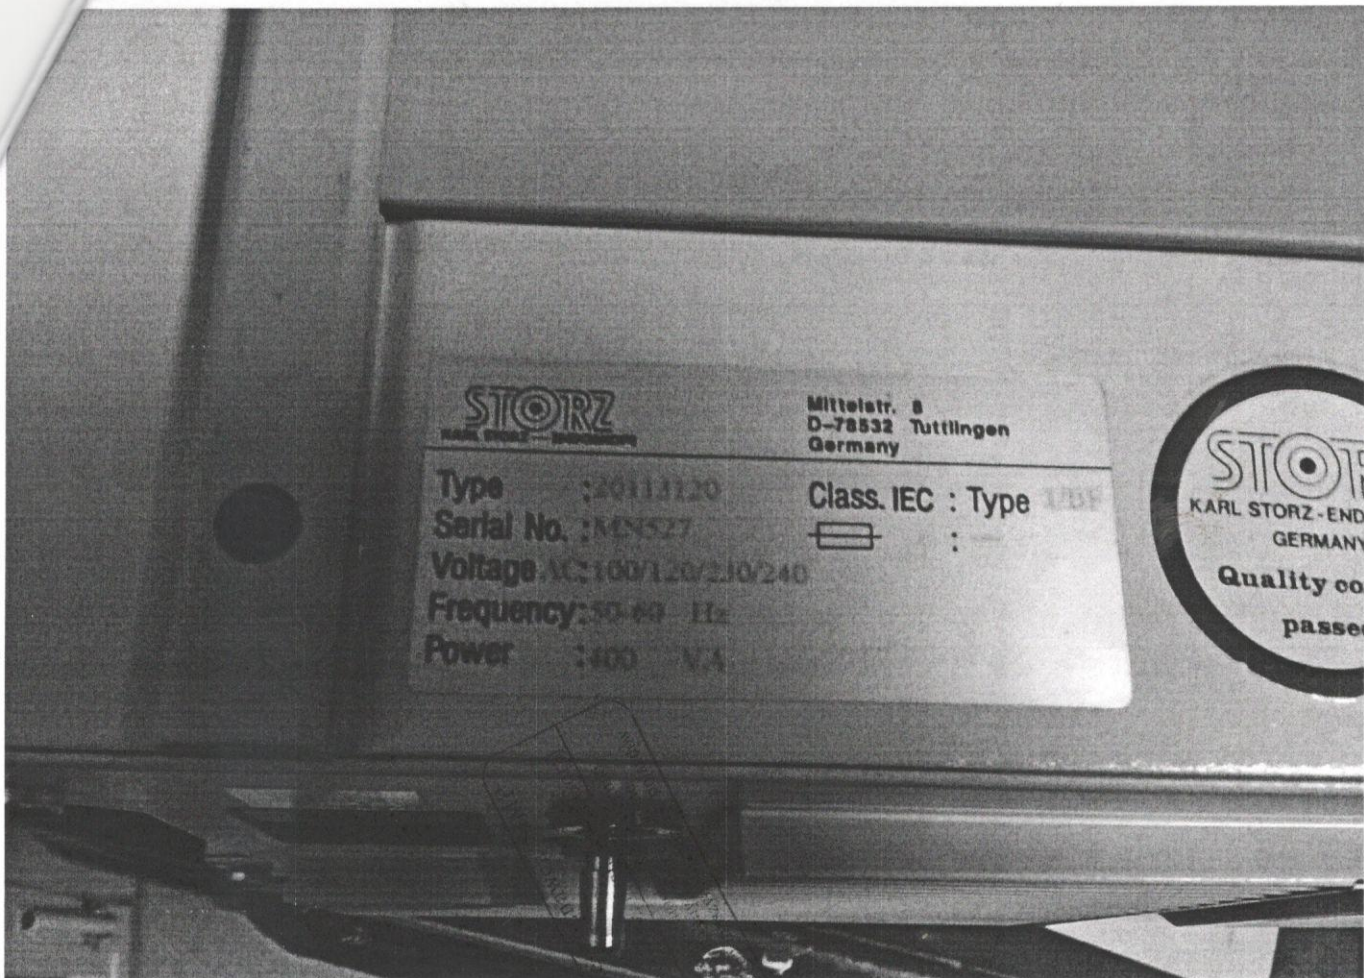

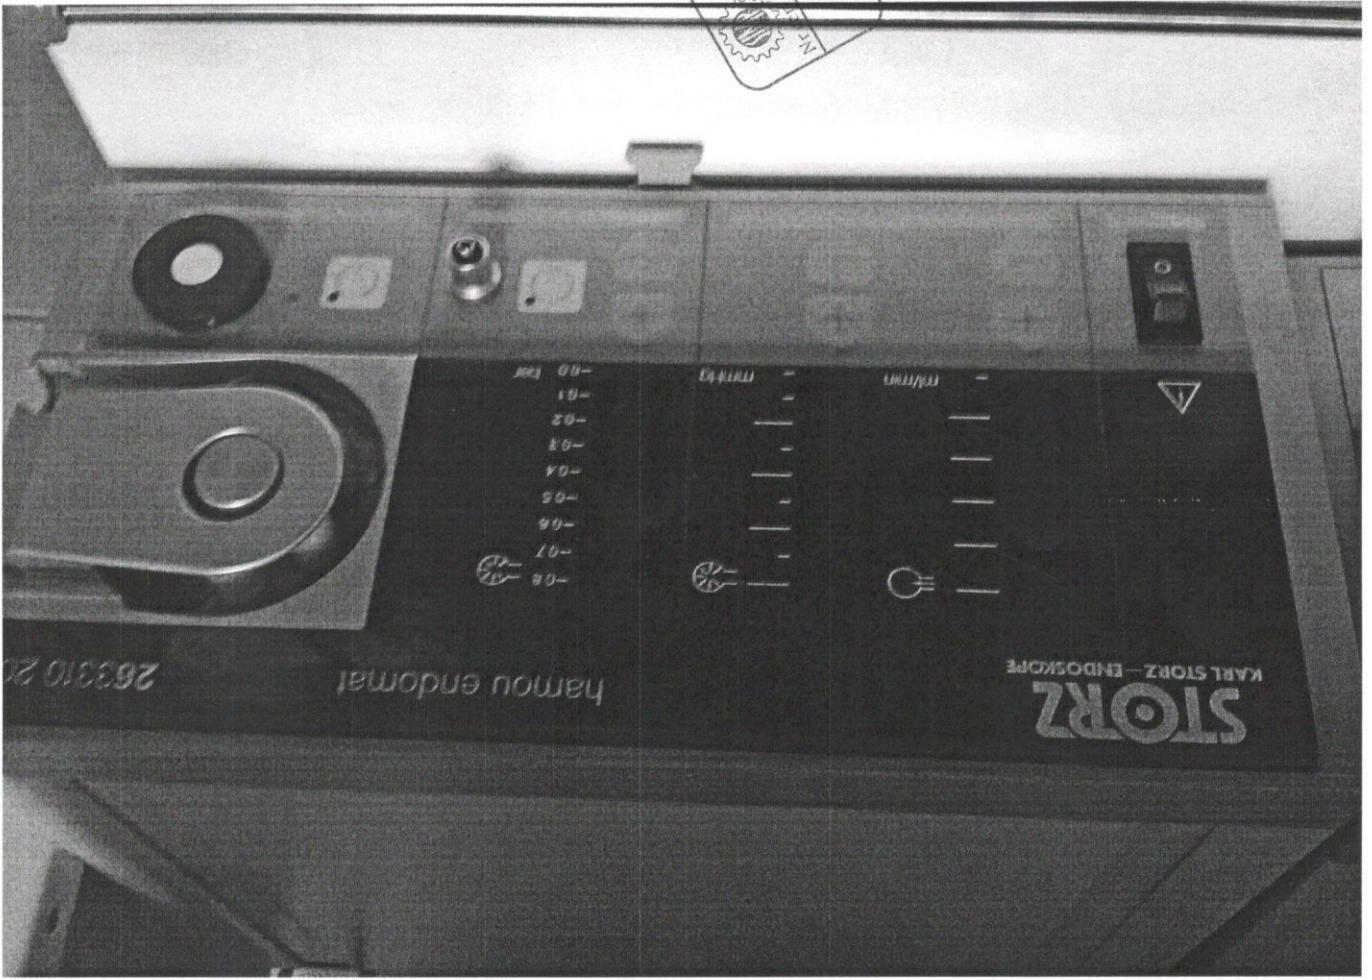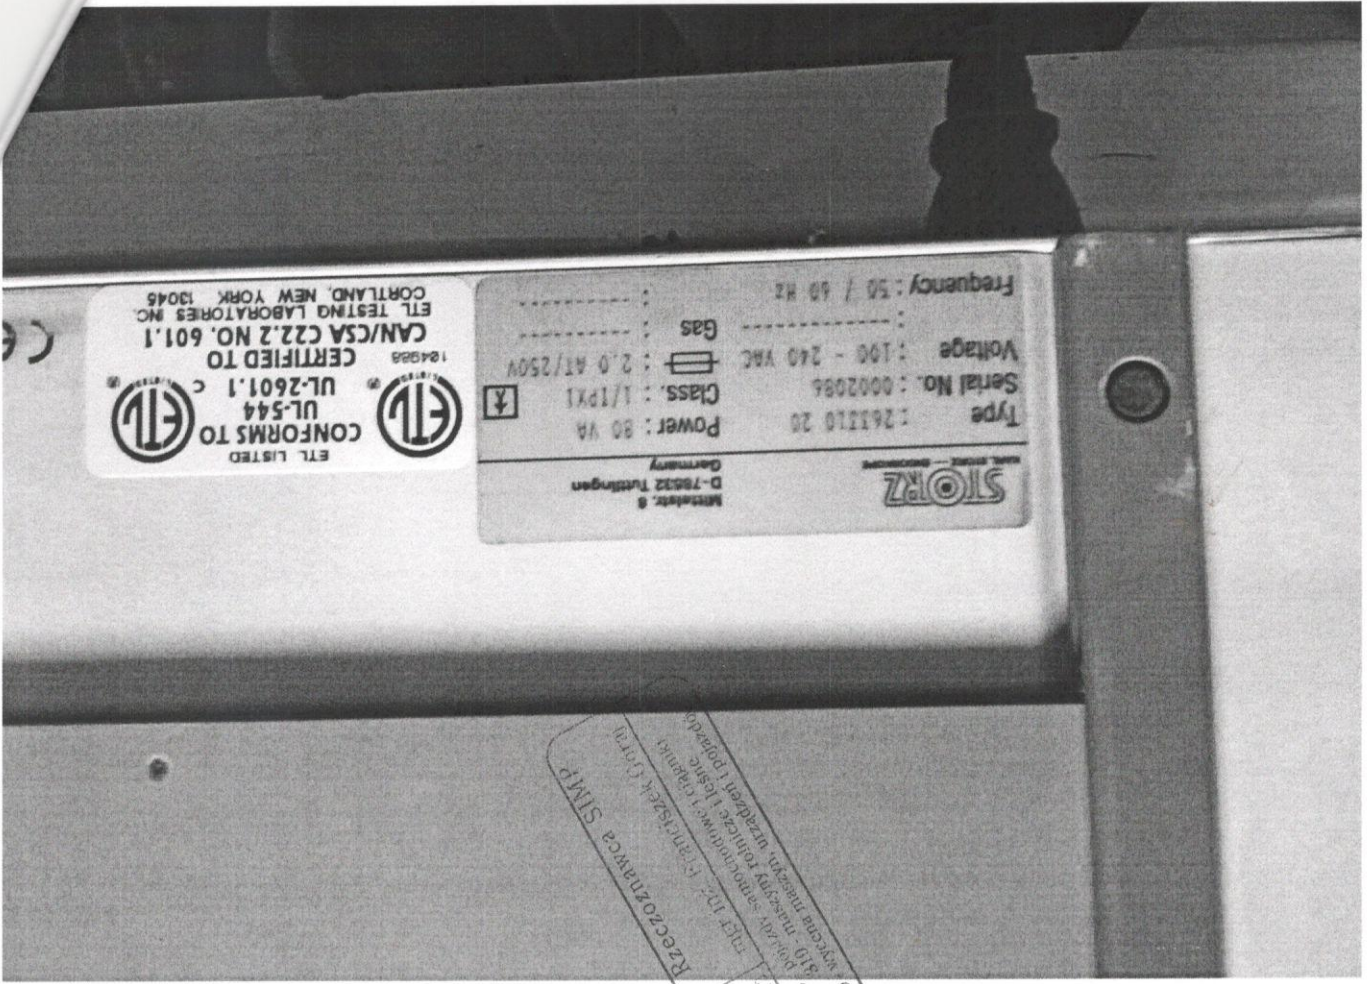


STORZ

KARL STORZ-ENDOSKOPF



Mittelstrasse 8
D-78532 Tuttlingen
Germany

Model: **20212020**
Voltage: **100 - 240 V-**
Frequency: **50/60 Hz**
Current: **0.5A**
Power: **40 W**

Classification IEC:
Class I
Type 



S/N: BM P010023

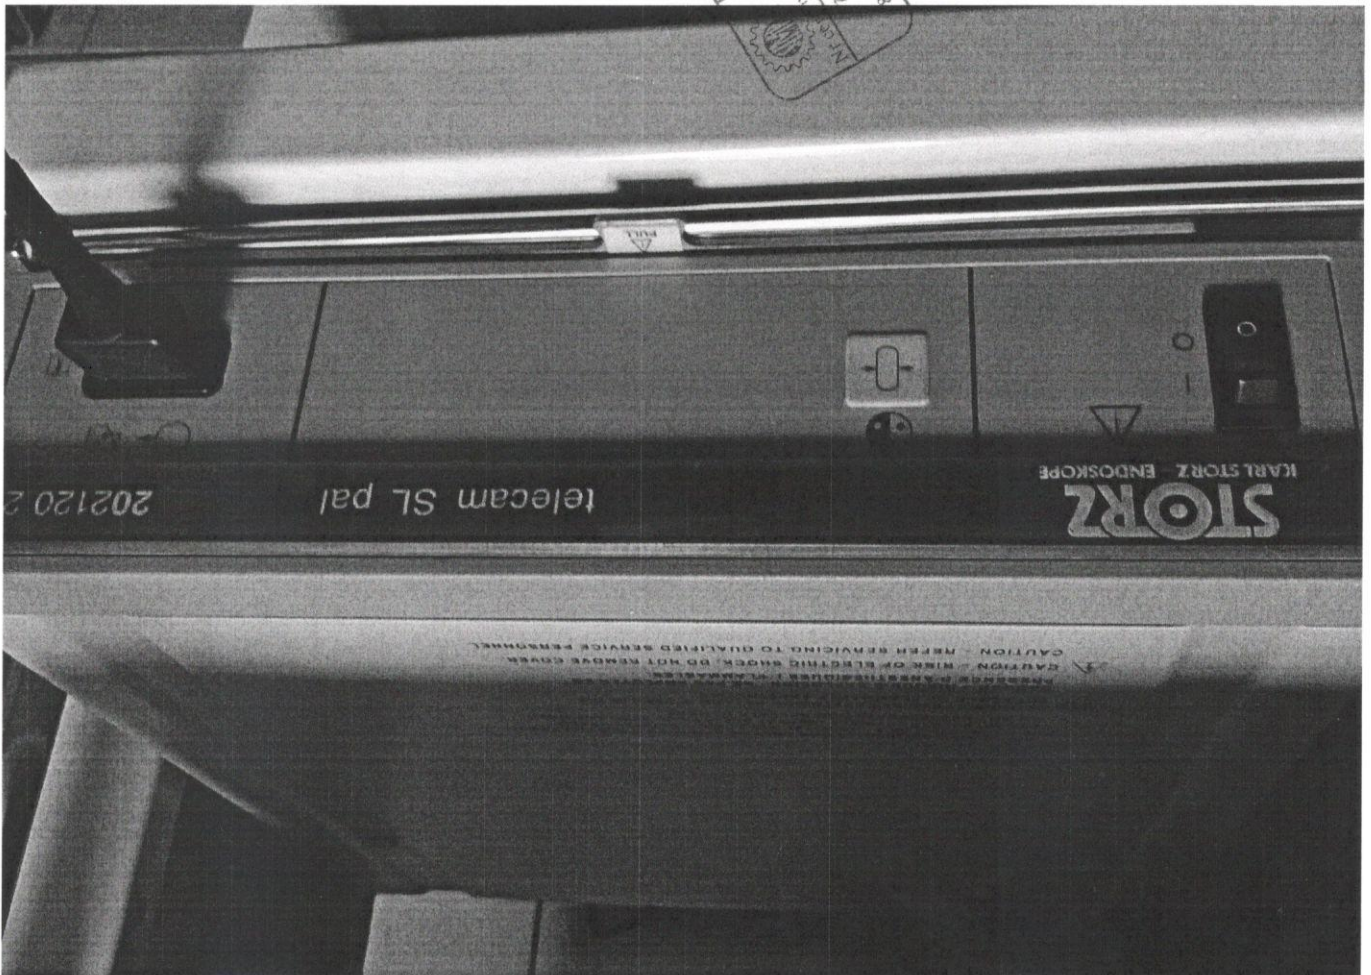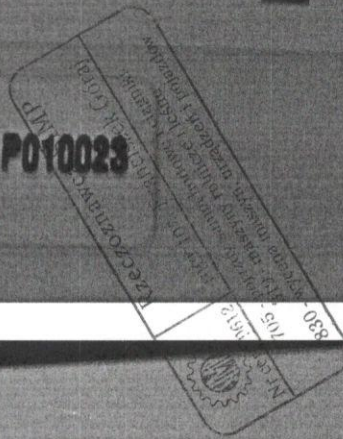

STORZ
L STORZ—ENDOSKOPE

electronic endoflator

264305 2

Control panel with two digital displays and various controls:

- Left display: Pressure measurement in mmHg, scale 0-50.
- Right display: Flow rate in l/min, scale 0-20.
- Buttons: Power, On/Off, and a large emergency stop button.
- Warning symbol: A triangle with an exclamation mark.
- Icons: A bottle, a person, and a hand.

Vertical stamp:
Rzecznik GOS
Wzrostowa 10
ul. ...
850-058

Technical specifications and certification labels:

- STORZ** logo and address: **Mittelstr. 8, D-78532 Tuttlingen, Germany**
- Type:** 264305 20
- Serial No.:** 0002011
- Voltage:** 100 - 240 VAC
- Class:** I / IPX1
- Power:** 180VA
- Gas:** CO 2
- Frequency:** 50 / 60 Hz
- ETL LISTED** logo and text: **CONFORMS TO UL-544 UL-2601.1 CERTIFIED TO CAN/CSA C22.2 NO. 601.1**
- ETL TESTING LABORATORIES INC**, **CORTLAND, NEW YORK 13045**

